


iBloodPressure®
Cellular Blood Pressure Monitor
Model SMBP802-GS-003
Model SMBP802-GS-004
User Manual

Arm Type

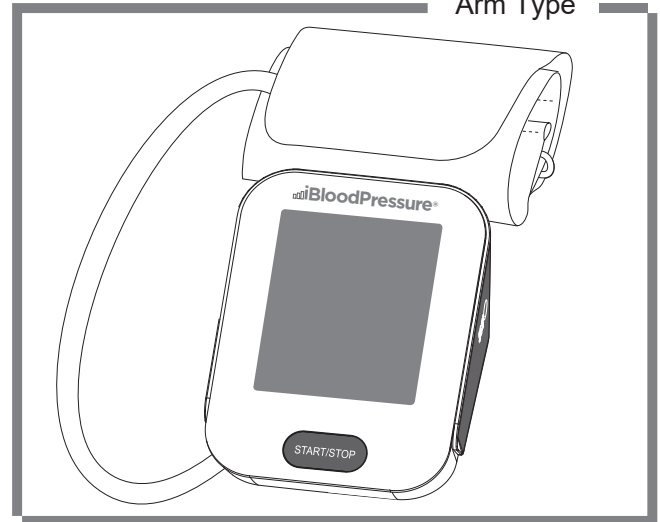

Manufactured for:
Smart Meter, LLC
5501 W. WATERS AVE., STE. 401
TAMPA, FLORIDA, 33634, UNITED STATES

B-O-UM-U-1022

To use the monitor correctly and safely, please read the manual thoroughly.
Please keep this manual for future reference.

Table of Contents

INTRODUCTION.....	2
• General Description	
• Receiving and Inspecting your Monitor	
• Indications for Use	
• Contraindications	
• Measurement Principle	
• Safety Information	
• LCD Display Signal	
• Components of the Device	
• What's Included	
BEFORE YOU START.....	9
• Choice of Power Supply	
• Installing and Replacing the Batteries	
MEASUREMENT.....	11
• Tie the Cuff	
• Taking a Measurement	
INFORMATION FOR USER.....	14
• Tips for measurement	
• Maintenances	
ABOUT BLOOD PRESSURE.....	16
• What are systolic pressure and diastolic pressure?	
• What is the standard blood pressure classification?	
• Irregular heartbeat detector	
• Why does my blood pressure fluctuate throughout the day?	
• Why do I get a different blood pressure at home compared to the hospital?	
• Is the result the same if measuring on the right arm?	
TROUBLESHOOTING	18
SPECIFICATIONS.....	19
EMC GUIDANCE.....	21
FCC STATEMENT.....	24
CONTACT INFORMATION.....	25

♥ General Description

The iBloodPressure® monitor features blood pressure measurement, pulse rate measurement, and cellular result transmission to cloud storage. Readings taken are equivalent to those obtained by a trained observer using the cuff and stethoscope auscultation method. This manual contains important safety and care information and provides step by step instructions for using the product. Read the manual thoroughly before using the product.

Patient is an intended operator.

Features:

- 78*92 mm Digital LCD display
- Measuring during inflation technology
- E-MTC wireless communication

♥ Receiving and Inspecting your Monitor

Remove this monitor from the packaging and inspect for damage. If this monitor is damaged, DO NOT USE and consult with your retail outlet or distributor.

♥ Indications for Use

The iBloodPressure® Blood Pressure Monitor is a digital monitor intended for use in measuring blood pressure and heartbeat rate with arm circumference ranging from 22cm to 45cm (about 8¾"-17½").

The device can be used to detect irregular heartbeat.

It is intended for adult indoor use only.

♥ Contraindications

1. Consult a medical professional before using this device if you have an implanted cardiac device, such as a pacemaker or defibrillator.
2. Consult a medical professional before using this device during pregnancy.

♥ Warranty

Smart Meter LLC warrants that this product will be free from defects in materials and workmanship for two years from the date of purchase.
















This warranty does not apply to the performance of an iBloodPressure® Meter that has been altered, misused, tampered with or abused in any way. This warranty applies only to the original purchaser of the iBloodPressure®. iBloodPressure® is a registered trademark of Smart Meter LLC.

♥ Measurement Principle

This product uses the Oscillometric Measuring Method to detect blood pressure. Before every measurement, the unit establishes a "zero point" equivalent to the atmospheric pressure. Then it starts inflating the cuff. Meanwhile, the unit detects pressure oscillation generated by beat-to-beat pulsatile, which is used to determine the systolic pressure and diastolic pressure as well as pulse rate.

♥ Safety Information

The signs below might be in the user manual, labeling or other components. They are the requirement of standard and using.

	Refer to instruction manual/booklet To signify that the instruction manual/ booklet must be read.(The background color of the symbol is blue.)		Type BF applied part
	Consult instructions for use or consult electronic instructions for use		Serial Number
	Direct Current		Polarity of d.c. power connector
	Class II Equipment		For indoor use only
	Batch code		Manufacturer
	Date of manufacture		General symbol for recovery/recyclable
	MR Unsafe To identify an item which poses unacceptable risks to the patient, medical staff or other persons within the MR environment.		
	Caution Indicates that caution is necessary when operating the device or control close to where the symbol is placed, or that the current situation needs operator awareness or operator action in order to avoid undesirable consequences.		
	The symbol indicates that the product should not be discarded as unsorted waste but must be sent to separate collection facilities for recovery and recycling.		

⚠ CAUTION

- * This device may be used only for the purpose described in this booklet. The manufacturer and Smart Meter cannot be held liable for damage caused by an incorrect application.

INTENDED USERS AND USES CAUTIONS

- * This device is intended for adult home use only.
- * This device is intended for non-invasive measuring and monitoring of arterial blood pressure. It is not intended for use on extremities other than the arm or for functions other than obtaining a blood pressure measurement.
- * Consult with your physician before using this monitor if you suffer from the following conditions: common arrhythmias such as premature ventricular beats or atrial fibrillation; peripheral arterial disease; pregnancy; preeclampsia; implantation with electrical devices; undergoing intravascular therapy; arteriovenous shunt or mastectomy. Please note that any of these conditions may affect measurement readings, in addition to patient motion, trembling or shivering.
- * The device is not suitable for measuring the blood pressure of children. Ask your doctor before using it on older children.
- * This device is not suitable for neonatal patients.
- * Do not confuse self-monitoring with self-diagnosis. This unit allows you to monitor your blood pressure. Do not begin or end medical treatment without asking a physician for treatment advice.
- * If you are taking medication, consult your physician to determine the most appropriate time to measure your blood pressure. Never change prescribed medication without consulting your physician.
- * Consult your doctor if you have any questions about your blood pressure.
- * When the device is used to measure patients who have common arrhythmias such as atrial or ventricular premature beats or atrial fibrillation, the best result may occur with deviation. Please consult your physician about the result.
- * Please report to the manufacturer and the competent authority of the Member State in which you are established about any serious incident that has occurred in relation to this device.
- * Do not apply the cuff on an arm that has other medical devices, an intravenous drip, or a blood transfusion attached.
- * Warning: Do not apply the cuff over a wound as it can cause further injury.
- * This device was clinically investigated according to the requirements of ISO 81060-2.

USE ENVIRONMENT CAUTIONS

- * Please use the device in the environment described in this manual. Otherwise, the performance and lifetime of the device will be reduced.
- * The device is intended for indoor home use.
- * The device is not intended for use during patient transport.
- * The device is not intended for public use.
- * The device cannot be used with HF surgical equipment at the same time.

⚠ CAUTION

- * The device is not AP/APG equipment and not suitable for use in the presence of a flammable anesthetic mixture with air of oxygen or nitrous oxide.
- * This unit is not suitable for continuous monitoring during medical emergencies or operations.
- * To avoid measurement errors, avoid electromagnetic field radiated interference signals or electrical fast transient/burst signals.
- * Wireless communications equipment such as wireless home network devices, mobile phones, cordless telephones and their base stations, and walkie-talkies may affect this equipment and should be kept at least 13 feet away from the device during use. The distance of 13 feet is calculated by the manufacturer from the 80 MHz to 5.8 GHz column of Table 4 and Table 9 of IEC 60601-1-2, as appropriate.
- * At least 30 minutes is required for the device to warm from the minimum storage temperature until it is ready for use. At least 30 minutes is required for the device to cool from the maximum storage temperature until it is ready for use.
- * The blood pressure monitor and the cuff are suitable for use within the home environment. If you are allergic to polyester, nylon, or plastic, please don't use this device.
- * During use, the patient will be in contact with the cuff. The materials of the cuff have been tested and found to comply with requirements of ISO 10993-5 and ISO 10993-10. The cuff should not cause irritation.

USE CAUTIONS


- * Too frequent and consecutive measurements could cause disturbances in blood circulation and injuries.
- * When using this device, please pay attention to the following situations which may interrupt blood flow and influence blood circulation and cause injury: connection tube kinking, too frequent and multiple consecutive measurements, the application of the cuff and pressurization on any arm with intravascular access therapy, where an arteriovenous (A-V) shunt is present, and inflating the cuff on the side of a mastectomy.
- * Don't compress, restrict, or kink the connection tube during use, otherwise, the cuff pressure may continuously increase which can prevent blood flow and result in injury.
- * Please check that operation of the device does not result in prolonged impairment of blood circulation.
- * If you experience discomfort during measurement, such as pain in the arm, press any button to release the air immediately from the cuff. Loosen the cuff and remove it from your arm.
- * If the cuff pressure reaches 40 kPa (300 mmHg), the unit will automatically deflate. Should the cuff not deflate when the pressure reaches 40 kPa (300 mmHg), detach the cuff from the arm immediately and press any button to stop inflation. Prolonged high pressure (cuff pressure > 300 mmHg or constant pressure > 15 mmHg for more than 3 minutes) applied to the arm may lead to an ecchymosis.
- * The operator should not touch the power supply and the patient simultaneously.

⚠ CAUTION

MAINTENANCE AND STORAGE CAUTIONS


- * This device contains sensitive components and must be treated with caution. Observe the storage and operating conditions described in this booklet.
- * When not in use, store the device in a dry room and protect it against extreme moisture, heat, lint, dust, and direct sunlight. Never place any heavy objects on the storage case.
- * Keep the unit out of reach of infants, young children, or pets to avoid inhalation or swallowing of small parts and possible strangulation from the hose or cable.
- * Cleaning: Dusty environments may affect the performance of the unit. Please use a soft cloth to clean the whole unit before and after use. Don't use abrasive or volatile cleaners.
- * Do not wash the cuff in a washing machine or dishwasher.
- * The service life of the cuff may vary by the frequency of washing, skin condition, and storage state. The typical service life is 10,000 uses.
- * Before use, make sure the device functions safely and is in proper working condition. Check the device and do not use the device if it is damaged in any way. The continuous use of a damaged unit may cause injury, improper results, or danger.
- * It is recommended that the performance of the device be checked every 2 years.
- * Please use only accessories and detachable parts specified/authorized by Smart Meter.
- * Please dispose of the device and accessories according to local guidelines.
- * Do not open or attempt to repair or service the device at any time.
- * If you have any questions or problems with this device, please contact Smart Meter Customer Service.

♥ LCD Display Signal

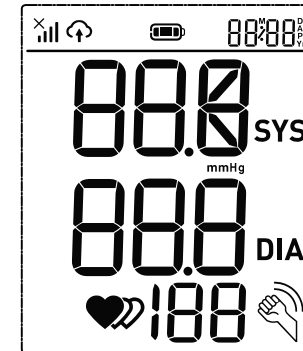

SYMBOL	DESCRIPTION	EXPLANATION
SYS	Systolic blood pressure	High pressure result
DIA	Diastolic blood pressure	Low pressure result
08:08 ^{PM}	Current Time	Time(year:month:day:hour:minute)
♥	Heartbeat	Heartbeat detection during measurement
mmHg	mmHg	Measurement Unit of the blood pressure
🔋	Battery Indicator	Indicate the current battery level
♥	Irregular heartbeat	Irregular heartbeat
🔄	Data transmission indication	Blinks to indicate that the data is being sent, the send success will disappear.
👏	Shaking reminder	Shaking will result in inaccurate result.
📶	Signal indication	Indicates the signal situation in the communication process.

♥ Components of the Device

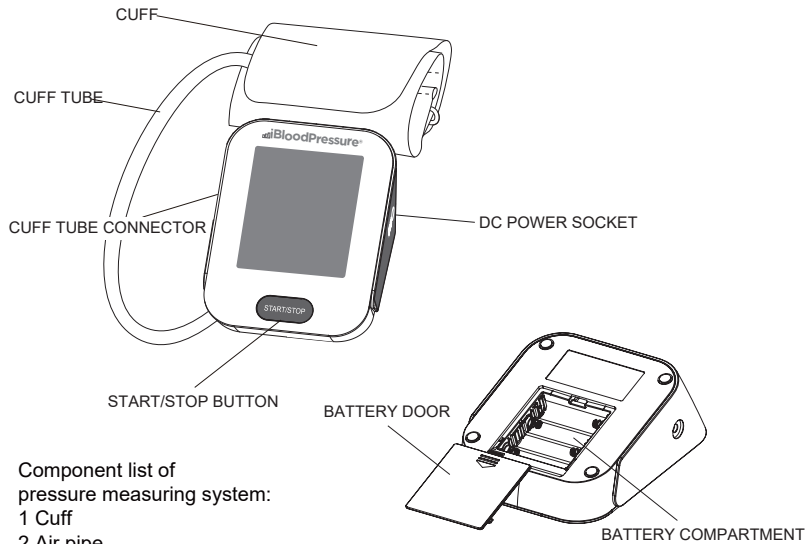

Component list of pressure measuring system:

- 1 Cuff
- 2 Air pipe
- 3 PCBA
- 4 Pump
- 5 Valve

♥ What's Included

1. Cellular Blood Pressure Monitor (SMBP802-GS-003 or SMBP802-GS-004)



3. User manual



2. Large Cuff 22-42cm – (AC2242-11) or Extra Large Cuff 22-45cm- (AC2245-021)




4. 4*AA batteries



♥ Choice of Power Supply

1. Battery powered mode:
6VDC 4*AA batteries
2. AC adapter powered mode:
6V \approx 1A (not included)
(Please use the AC adapter which is authorized by the manufacturer!)

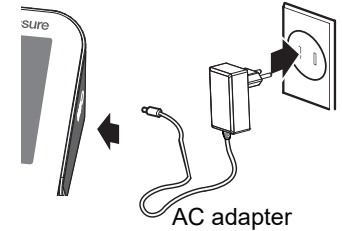


⚠ CAUTION

In order to get the best effect and protect your monitor, please use the right batteries and special power adapter which complies with local safety standards.

♥ Installing and Replacing the Batteries

If this is your first time using the device:

1. Slide open the battery door on the back of the device.
2. Install the batteries provided with the device. Follow the diagram inside the battery compartment for correct polarity—the springs should align with the negative sign on the batteries.
3. Slide the battery door closed.





Replace the batteries whenever the below happens

- The shows
- The display dims
- The display does not light up



⚠ CAUTION


- Do not use new and used batteries together.
- Do not use different types of batteries together.
- Do not dispose of the batteries in fire. Batteries may explode or leak.
- Remove batteries if the device is not likely to be used for some time.
- Worn batteries are harmful to the environment. Do not dispose with daily garbage.
- Remove the old batteries from the device following your local recycling guidelines.


Tip:

When you replace the batteries or connect the AC adapter, the symbol  and  will be shown on the LCD, indicating pair-up is proceeding alternatively.

You can press “ START/STOP ” button at any time to stop pair-up.




If **SUCCEED**, symbol  will be shown on the LCD.



If **FAIL**, the monitor will turn off automatically.

♥ Tie the Cuff

1. Plug the connector on cuff tube into the device.
2. Expose your upper arm by removing or adjusting clothing and jewelry. Make sure blood flow is not constricted by a rolled up sleeve.
3. Open the cuff and loosen fully.
4. Orient the cuff so that the tube exits towards the hand.
5. Place your arm through the cuff loop, with your palm facing up.
6. Position the cuff's edge about an inch (2–3 cm) above the elbow.
7. Align the Φ marker (located to the right of the tube exit) with the center of your arm.
8. Tighten the cuff evenly around your arm by pulling on the end—make sure the Φ marker stays aligned with the center of your arm.
9. Wrap the end of the cuff over your arm to secure it in place. Don't make it too tight—allow a finger to fit between the cuff and your arm.
10. If possible, relax and rest for at least 5 minutes before taking a measurement.
11. Lay your arm on a table with your palm facing up. The cuff should be at the same height as your heart. Sit up straight and rest your feet flat on the ground. Make sure the tube is not kinked or pinched.

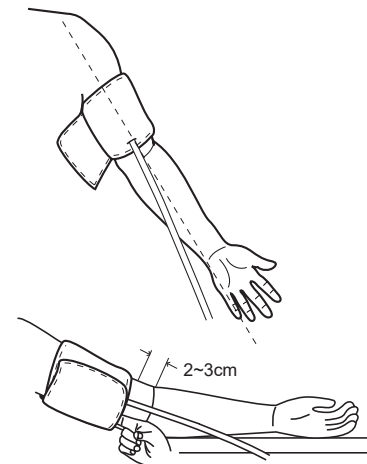

♥ Taking a Measurement


1. When the monitor is off, press the “ START/STOP ” button to turn on the monitor. The cuff will automatically inflate, complete the measurement, and transmit the results.




LCD display




Inflating and measuring.




Display resets to zero.






Display the results.




Transmitting results.




2. The device will transmit the data after measurement. The symbol  blinks on the LCD indicating data is transmitting.

3. If the data is successfully transmitted, the symbol  will disappear and the LCD will display  and then the device will turn off automatically.



If the data transmission fails, Error message will be shown (take E6 for example) on the display for several seconds then the device will turn off automatically.

Note: the result will be transmitted next time a cellular connection is made.



Tip:

You can press “ START/STOP ” button at any time to stop measuring during the process.

♥ Tips for Measurement

Measurements may be inaccurate if taken in the following circumstances.



Within 1 hour
after dinner or drinking



Immediately after
tea, coffee, smoking



Within 20 minutes
after taking a bath



When talking or moving
your hands



In a very cold environment




When you need to urinate




♥ Maintenance


To get the best performance, please follow the steps below.



Store in a dry place and avoid the sunshine




Avoid intense shaking
and dropping




Use a damp cloth to remove dirt



Avoid contact with water,
clean exterior with a dry cloth

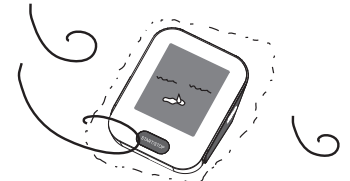


Avoid dusty places and
unstable temperatures



Avoid washing the cuff

♥ What are systolic pressure and diastolic pressure?

When ventricles contract and pump blood out of the heart, the blood pressure reaches its maximum value in the cycle, which is called systolic pressure. When the ventricles relax, the blood pressure reaches its minimum value in the cycle, which is called diastolic pressure.



♥ What is the standard blood pressure classification?

The chart on the right is the standard blood pressure classification published by American Heart Association (AHA).

This chart reflects blood pressure categories defined by American Heart Association.

Blood Pressure Category	Systolic mmHg (upper#)		Diastolic mmHg (lower#)
Normal	less than 120	and	less than 80
Prehypertension	120-129	and	less than 80
High Blood Pressure (Hypertension) Stage 1	130-139	or	80-89
High Blood Pressure (Hypertension) Stage 2	140 or higher	or	90 or higher
Hypertensive Crisis (Consult your doctor immediately)	Higher than 180	and/or	Higher than 120

⚠ CAUTION

Please consult a physician if your result falls outside the range. Please note that only a physician can tell whether your blood pressure value has reached a dangerous point.

♥ Irregular Heartbeat Detector

An irregular heartbeat is detected when a heartbeat rhythm varies while the device is measuring systolic pressure and diastolic pressure. During each measurement, the blood pressure monitor will keep a record of all the pulse intervals and calculate their average value. If there are two or more pulse intervals with an average difference between each interval of more than $\pm 25\%$, or if there are four or more pulse intervals, with an average difference between each interval of $\pm 15\%$, then the irregular heartbeat symbol will appear on the display with the measurement result.

⚠ CAUTION

The appearance of the IHB icon indicates that a pulse irregularity consistent with an irregular heartbeat was detected during measurement. Typically this is NOT a cause for concern. However, if the symbol appears often, we recommend you seek medical advice. Please note that the device does not replace a cardiac examination, but serves to detect pulse irregularities at an early stage.

♥ Why does my blood pressure fluctuate throughout the day?

1. Individual blood pressure varies throughout the day. It is also affected by the way you tie your cuff and your measurement position. It is recommended that you take your measurement under the same conditions.
2. If you take medicine, your pressure may vary more.
3. Wait at least 3 minutes between measurements.

♥ Why do I get a different blood pressure at home compared to the hospital?

The blood pressure is different throughout the day due to weather, emotion, exercise, etc. Also, there is the “white coat” effect, which means blood pressure usually increases in clinical settings.


♥ Is the result the same if measuring on the right arm?

It is okay to measure on either arm, however; there may be different results for some people. We suggest you measure the same arm every time.

♥ Pay special attention to the following when you measure your blood pressure at home:

- If the cuff is tied properly.
- If the cuff is too tight or too loose.
- If the cuff is tied on the upper arm.
- If you feel anxious.
- Take 2-3 deep breaths before you begin measuring.
- Relax for 4-5 minutes until you are calm.

This section includes a list of error messages and frequently asked questions for issues you may encounter with your blood pressure monitor.

PROBLEM	SYMPTOM	CHECK THIS	REMEDY
No power or Low batteries	Display will not light up or  shows	Batteries are exhausted.	Replace with new batteries.
		Batteries are inserted incorrectly.	Insert the batteries correctly.
		AC adapter is inserted incorrectly.	Insert the AC adapter tightly.
Error message	E 1 shows	The cuff is not secure or abnormal inflation.	Refasten the cuff and then measure again.
	E 2 shows	The monitor detected the motion, talking or the pluse is too weak while measuring.	Movement can affect the measurement. Relax for a moment and then measure again.
	E 3 shows	The measurement process does not detect the pulse signal.	Loosen the clothing on the arm and then measure again.
	E 4 shows	Not able to calculate, measurement failed.	Relax for a moment and then measure again.
	E 5 shows	Failed to communicate with the server.	Contact customer service.
	E 6 shows	No access to network.	Contact customer service.
	EExx, shows on the display.	A calibration error occurred.	Retake the measurement. If the problem persists, contact customer service for further assistance. Refer to the warranty for contact information and return instructions.
Warning message	Out shows	Out of measurement range.	Relax for a moment. Refasten the cuff and then measure again. If the problem persists, contact your physician.

External dimensions	Approx. 154.3 mm*121.5 mm*68.1 mm
Display mode	Digital LCD V.A. 78 mm*92 mm
Weight	Approx. 393g (Excluding the batteries)
Measurement mode	Oscillographic testing mode
Mode of operation	Continuous operation
Measurement range	Rated cuff pressure: 0 mmHg ~ 299 mmHg (0 kPa ~ 39.9 kPa) Measurement pressure: SYS: 60 mmHg ~ 230 mmHg (8.0 kPa ~ 30.7 kPa) DIA: 40 mmHg ~ 130 mmHg (5.3 kPa ~ 17.3 kPa) Pulse value: (40-199) beat/minute
Accuracy	Pressure: within ± 3 mmHg (0.4 kPa) Pulse value: $\pm 5\%$
Power supply	Battery powered mode: 6VDC 4*AA batteries AC adapter powered mode: 6V $\overline{\text{---}}$ 1A (not included) (Please only use the recommended AC adapter).
Measurement perimeter of the upper arm	22 cm~45 cm
Attachment	4*AA batteries, user manual
Mobility	Hand held medical device to be used on a resting patient.
Type of use/reuse	Multiple patient multiple use
Degree of protection	Type BF applied part

Protection against water ingress	IP21: It means the device could be protected against solid foreign objects of 12,5mm Φ and greater, and against vertically falling water drops.
Device Classification	Battery Powered Mode: Internally Powered ME Equipment AC Adapter Powered Mode: Class II ME Equipment
General Environment	- home use, not intended for professional use - indoor use only - not for use in shower, bath tub or sink
Normal working condition	A temperature range of: +5°C to +40°C A relative humidity range of 15% to 90%, non-condensing, but not requiring a water vapour partial pressure greater than 50 hPa An atmospheric pressure range of: 700 hPa to 1060 hPa
Storage & transportation condition	Temperature: -20°C to +60°C A relative humidity range of \leq 93%, non-condensing, at a water vapour pressure up to 50 hPa
Conditions of visibility	Ambient luminance range: 100 lx to 1500 lx
Background sound pressure level	\leq 50 dB in the range of 100 Hz — 8 kHz
Software Version	A01
Service life	2 years

WARNING: No modification of this equipment is allowed.

♥ EMC Guidance

The ME EQUIPMENT or ME SYSTEM is suitable for home healthcare environments

Warning: Do not use near active HF surgical equipment and the RF shielded room of an ME system for magnetic resonance imaging, where the intensity of EM disturbances is high.

Warning: Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

Warning: Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

Warning: Portable RF communications equipment (including peripherals such as antenna cables and external external antennas) should be used no closer than 30 cm (12 inches) to any part of the equipment SMBP802-GS-003 or SMBP802-GS-004, including cables. Otherwise, degradation of the performance of this equipment could result.

Technical description:

- 1, All necessary instructions for maintaining BASIC SAFETY and ESSENTIAL PERFORMANCE with regard to electromagnetic disturbances for the expected service life.
- 2, Guidance and manufacturer's declaration -electromagnetic emissions and immunity

Table 1

Guidance and manufacturer's declaration - electromagnetic emissions	
Emissions test	Compliance
RF emissions CISPR 11	Group 1
RF emissions CISPR 11	Class [B]
Harmonic emissions IEC 61000-3-2	Class A
Voltage fluctuations/ flicker emissions IEC 61000-3-3	Comply

Table 2

Guidance and manufacturer's declaration – electromagnetic Immunity		
Immunity Test	IEC 60601-1-2 Test level	Compliance level
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air
Electrical fast transient/burst IEC 61000-4-4	±1 kV ±2 kV, 100 kHz repetition frequency	For AC power port: Power supply lines: ±2 kV
Surge IEC61000-4-5	±1 kV (Line to ±0.5 kV line) ±0.5 kV ±1 kV ±2 kV (Line to ground) ±2 kV Signal line (LAN line)	For AC power port: Line to lines: ±1 kV
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	0%, 70%, 0% of UT	For AC power port: 0 % for 0,5 cycle, 0% for 1 cycle 70 % for 25 cycles; Single phase: 0% for 250 cycle
Power frequency magnetic field IEC 61000-4-8	30 A/m 50 Hz/60 Hz	30 A/m 50 Hz/60 Hz
Conducted RF IEC61000-4-6	0,15 MHz – 80 MHz 3V ISM and amateur radio bands between 0,15 MHz and 80 MHz 6V	For AC power port: 3 Vrms 6 Vrms (in ISM and amateur radio bands) 80% AM at 1 KHz
Radiated RF IEC61000-4-3	10 V/m 80 MHz – 2,7 GHz 80 % AM at 1 kHz	10 V/m 80 MHz – 2,7 GHz 80% AM at 1 kHz
NOTE UT is the a.c. mains voltage prior to application of the test level.		

Table 3

Guidance and manufacturer's declaration - electromagnetic Immunity								
Radiated RF IEC61000-4-3 (Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment)	Test Frequency (MHz)	Band (MHz)	Service	Modulation	Maximum Power (W)	Distance (m)	IEC 60601-1-2 Test Level (V/m)	Compliance level (V/m)
	385	380-390	TETRA 400	Pulse modulation 18 Hz	1.8	0.3	27	27
	450	430-470	GMRS 460, FRS 460	FM ± 5k Hz deviation 1 kHz sine	2	0.3	28	28
	710	704-787	LTE Band 13, 17	Pulse modulation 217 Hz	0.2	0.3	9	9
	745							
	780							
	810	800-960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation 18 Hz	2	0.3	28	28
	870							
	930							
	1720	1700-1990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3, 4, 25; UMTS	Pulse modulation 217 Hz	2	0.3	28	28
	1845							
	1970							
	2450	2400-2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation 217 Hz	2	0.3	28	28
	5240	5100-5800	WLAN 802.11 a/n	Pulse modulation 217 Hz	0.2	0.3	9	9
5500								
5785								

♥ FCC Statement

FCC ID: OU9LS802GSM2

This device complies with Part 15 of the FCC Rules. Operation is subject to the two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Caution: The user is cautioned that changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation.

If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:


- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

FCC Radiation Exposure Statement:

To maintain compliance with the FCC's RF Exposure guidelines, this equipment should be installed and operated with a minimum distance of 20 cm from your body: Use only the supplied antenna.

♥ Authorized Components

1. Please use the iBloodPressure® authorized adapter (not included).

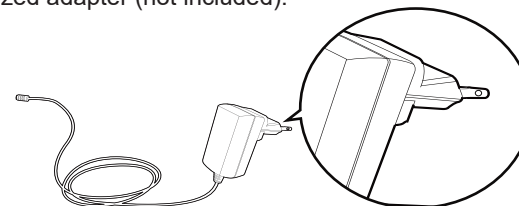


Adapter

Type: BLJ06L060100P-U

Input: 100-240 V, 50-60 Hz, 0.2 A max

Output: 6V \equiv 1000 mA

2. Please use authorized iBloodPressure® cuffs only
Large Cuff 22-42cm – (AC2242-11) or
Extra Large Cuff 22-45cm- (AC2245-021)



♥ Contact Information

Manufactured for: Smart Meter, LLC

Company: Smart Meter, LLC

Address: 5501 W. WATERS AVE., STE. 401
TAMPA, FLORIDA, 33634, UNITED STATES
www.smartmeterrpm.com
Toll Free Customer Support:
1-844-445-8267
Mon-Fri 9am-5pm ET